

# Accurate and Efficient Frequency Evaluation of a Ring Oscillator

Application Note 4070-3

## Agilent 4070 Series of Semiconductor Parametric Testers

### Introduction

With the continued demand for higher-speed operation of semiconductor devices, the measurement of gate delay and interconnect delay has become more important than ever. These two parameters play key roles in determining the ultimate speed of device operation. High-speed operation has always been critical for successful logic devices. With new market pressures on peripheral devices, the need for high-speed operation is now becoming necessary for memory devices.

It is commonly known that gate delay time can be evaluated by measuring the oscillation frequency of a ring oscillator test structure.

Interconnect delay, which is becoming significant for devices designed with less than 0.8  $\mu\text{m}$  gate length, can also be evaluated using a specially designed ring oscillator test structure.

Because of this, measurement of the oscillation frequency of a ring oscillator has become an indispensable tool for semiconductor device engineers when designing high-speed devices.

This measurement can also be used to determine if devices are fabricated as designed, or to model AC characteristics by supplying measured data to simulation software. Today, measurement of the frequency of the ring oscillator is feasible on the production line. This application note introduces a precise and fast measurement method to measure the oscillation frequency of a ring oscillator structure using a spectrum analyzer integrated into the Agilent 4072A Advanced Parametric Tester.

### Conventional Testing Methods

The objective of measuring the ring oscillator's frequency is to obtain the gate delay time. This can be calculated from the following equation:

$$t_{pLH} + t_{pHL} = \frac{1}{(2n + 1) \cdot \text{freq}}$$

freq: Oscillation frequency

2n+1: Number of stages (or inverters)

$t_{pLH}$ : Gate delay time for the output to change from low to high

$t_{pHL}$ : Gate delay time for the output to change from high to low


If a test structure consisting of a ring oscillator and long interconnect line is used, the interconnect delay can also be evaluated by comparing the result with another test structure that consists of only a ring oscillator. Often a bench-top frequency counter or oscilloscope connected to a manual probe station is used to measure the oscillation frequency of a ring oscillator. The frequency counter solution has the advantage of lower cost and higher measurement speed. However, there are some disadvantages.

- The frequency counter cannot detect waveform distortion caused by the device itself or by the measurement test system, so the measured result can be less reliable.
- It may pick up harmonics.
- If there is an offset voltage present, the frequency counter cannot accurately measure zero crossings.



**Agilent Technologies**

Innovating the HP Way

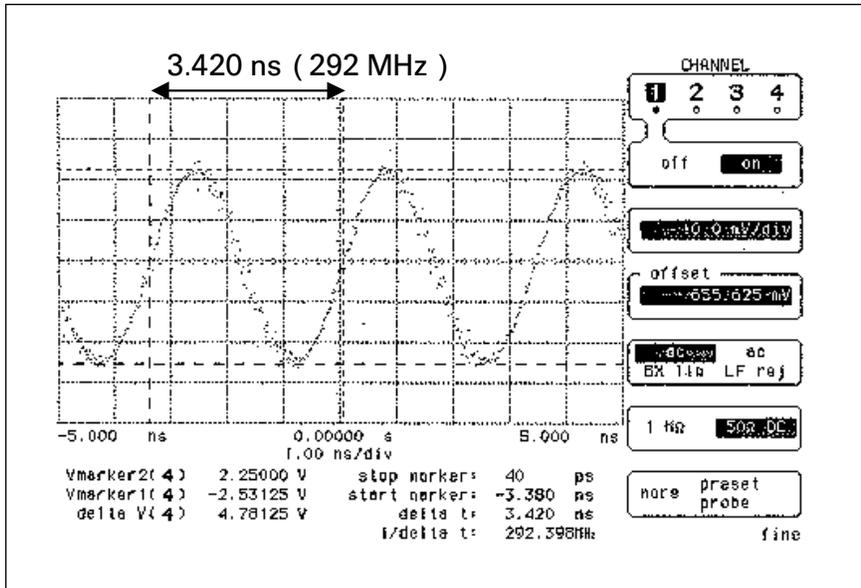

**Figure 1. Waveform of a ring oscillator through the switching matrix of the Agilent 4072A Parametric Tester**

The oscilloscope solution is reliable because the actual waveform can be monitored. However, there are also some disadvantages with this method.

- The measurement and analysis speed is slow.
- In a fully automated measurement system, it may return an incorrect frequency due to waveform distortion.
- The cost is high.

The oscilloscope solution is good for a measurement when using a manual probe station because the signal loss or distortion caused by the measurement path is small. However, if integrated into an automatic test system that includes a switching matrix, an oscilloscope is no longer a suitable solution due to the waveform distortion at higher frequencies.

If a parametric tester, integrated with a frequency counter or an oscilloscope, is used for the evaluation, the design of the test structure has to be considered as well. To minimize the waveform distortion caused by the switching matrix, the oscillation frequency needs to be reduced. Therefore, the area of the test structure can become very large due to the increased number of stages required to reduce the frequency of oscillation. For example, to reduce the oscillation frequency from 100 MHz to 10 MHz, the area of the ring oscillator increases by about ten times, using up precious space on a wafer.

**Solution Using the Agilent 4072A and a Spectrum Analyzer**

The 4072A Advanced Parametric Tester reduces one of the bottlenecks that prevent a semiconductor parametric tester from being used for this application.

The HF (High Frequency) port of the 4072A has outstanding high frequency characteristics.

An oscilloscope output of an actual ring oscillator output waveform monitored through the switching matrix of the 4072A is shown in Figure 1. The successful monitoring of an oscillation frequency that is close to 300 MHz is displayed.

Utilizing the superior frequency characteristics of the 4072A will reduce many of the difficulties of ring oscillator evaluation.

A spectrum analyzer can be integrated in the 4072A and used to measure the frequency of the ring oscillator. A spectrum analyzer with a reasonably wide frequency range, such as 1.5 GHz, is recommended. The spectrum analyzer is used in the system to directly measure the highest amplitude frequency, which should correspond to the oscillation frequency of the ring oscillator. There are several benefits that make a spectrum analyzer suitable for this application.

- Measurement speed is fast.
- The oscillation frequency can be precisely measured in the presence of an offset voltage.
- The usable frequency range is higher due to the wide baseband frequency range of the spectrum analyzer.
- The cost is reasonable.

Most Agilent spectrum analyzers have marker peak detection functions and GPIB control capability. These are both essential for configuring an automated measurement system.

Figure 2 shows an example measurement program using the TIS (Test Instruction Set) commands of the parametric tester and a custom driver for a spectrum analyzer.

```

1000 OPTION BASE 1
1010 INTEGER Spana
1011 INTEGER Ro, Buf, Out, Rognd
1020 !
1060 Spana=2718          ! GPIB Address
1070 Minf=1.00E+8       ! Sweep start frequency
1080 Maxf=900E+8        ! Sweep stop frequency
1090 Rbw=1.E+6          ! Resolution band width
1100 N=101              ! Number of inverters in the R.O.
1110 Fcr=1.00E+4        ! Frequency counter resolution
1111 !
1112 Vcc=3.3            ! Drive voltage
1113 Icomp=4.00E-2      ! Current compliance
1114 !
1115 Ro=2               ! Pin assignment
1116 Buf=4              !
1117 Rognd=6           !
1118 Out=8              !
1120 !
1121 Init_system       ! Initializes Agilent 4072A
1130 Init_spa(Spana)  ! Initializes E4411A
1131 !
1133 Connect(FNPort(1,9),Rognd) ! Connection
1134 Connect(FNPort(3,1),Out)    !
1135 Connect(FNPort(1,2),Ro,Buf) !
1136 Force_v(Ro,Vcc,Vcc, Icomp) ! Drive R.O.
1140 Set_spa(Minf, Maxf ,Rbw)    ! Set up measurement
1150 Measure_spa(Osc_freq,Amp,Delay,N,Fcr) ! Measure osc. frequency
1170 Disable_spa
1180 Disable_port
1190 Connect
1191 !
1200 PRINT "Freq: ";Osc_freq;"(Hz), Gate delay: ";Delay;"(s)"
1210 END

```

*Italic* : Spectrum analyzer control  
**Bold** : Agilent 4072A's TIS command

Further measurements can be performed in order to get better accuracy if a marker frequency counter function is available on the spectrum analyzer. Unlike a frequency counter, a spectrum analyzer will not return an incorrect value by counting a harmonic of the ring oscillator.

Figure 3 shows example frequency measurement results of actual ring oscillators.

The characteristics shown in Figure 3 (A) were measured on the same device as shown in Figure 1. The results of the frequency measurements are nearly identical.

The connection diagram required for this measurement is shown in Figure 4.

Figure 2. Measurement program example


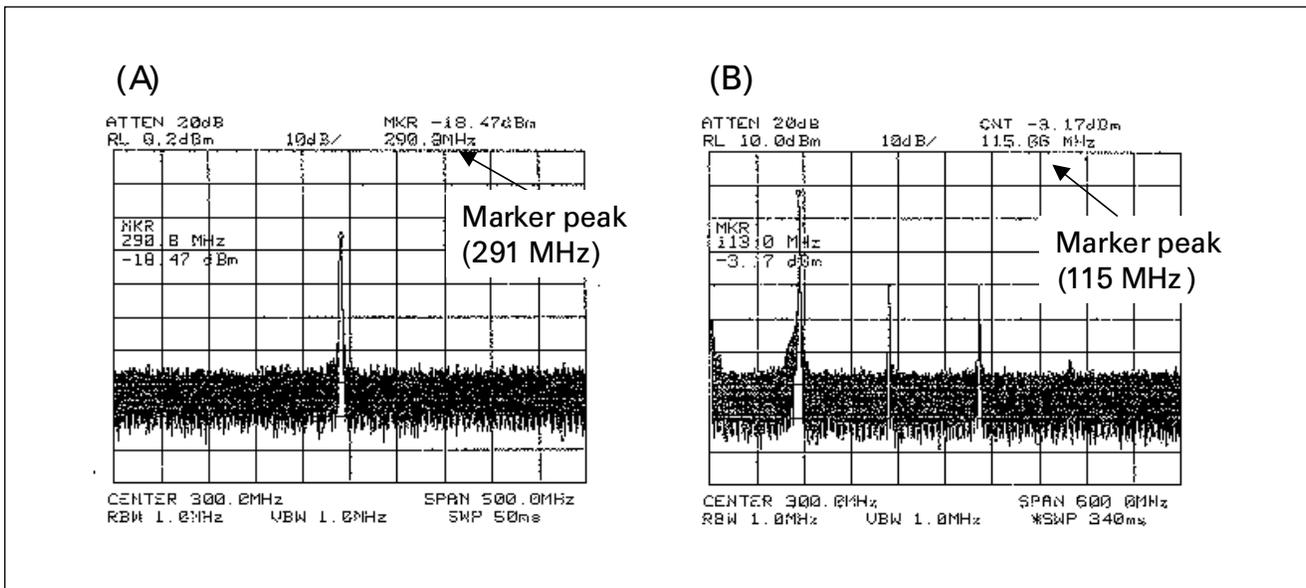


Figure 3. Example of ring oscillator evaluation results at 291 MHz (A) and 115 MHz (B)

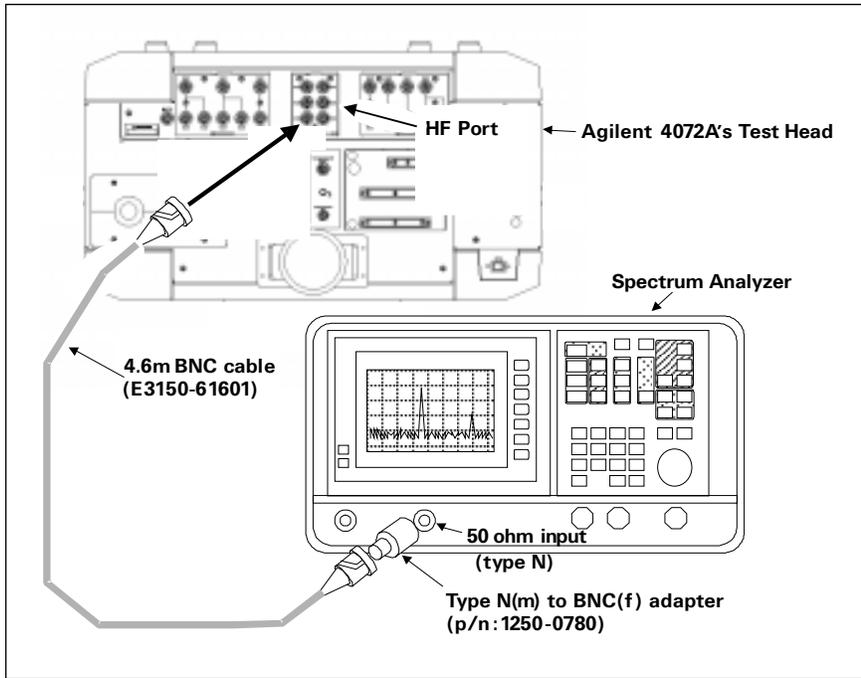

**Figure 4. Measurement program example**

**Conclusion**

Gate delay and interconnect delay, both of which are critical parameters in the sub-micron device era, can efficiently be evaluated using the Agilent 4072A Parametric Tester and a spectrum analyzer. Automatic evaluation allows collection of a reasonable amount of data both in R&D during design, and in production for advanced analysis and process monitoring.

For more information about Agilent Technologies semiconductor test products, applications, and services, visit our website: [www.agilent.com/go/semiconductor](http://www.agilent.com/go/semiconductor) or you can call one of the centers listed and ask to speak with a semiconductor test sales representative.

For more information about other Agilent test and measurement products, go to [www.agilent.com](http://www.agilent.com)

**United States:**  
1 800 452 4844

**Canada:**  
1 877 894 4414

**Europe:**  
(31 20) 547 2000

**Japan:**  
(81) 426 56 7832  
Fax: (81) 426 56 7840

**Latin America:**  
(305) 269 7500  
Fax: (305) 269 7599

**Australia/New Zealand:**  
1 800 629 485 (Australia)  
Fax: (61 3) 9272 0749  
0 800 738 378 (New Zealand)  
Fax: (64 4) 495 8950

**Asia Pacific:**  
(852) 2599 7889  
Fax: (852) 2506 9233

**Taiwan:**  
(886 2) 717 9524  
Fax: (886) 2 718 9860

**Korea:**  
(822) 769 0800  
Fax: (822) 786 1083

**Singapore:**  
(65) 1 800 292 8100  
Fax: (65) 275 0387

Product specifications and descriptions in this document subject to change without notice.

Copyright © 2000 Agilent Technologies  
Printed in U.S.A. 11/00  
5968-4310E



**Agilent Technologies**

Innovating the HP Way