

# Customizing Agilent B1500A EasyEXPERT Application Tests

Application Note B1500-4

## Agilent B1500A Semiconductor Device Analyzer

### Introduction


The Agilent B1500A Semiconductor Device Analyzer with EasyEXPERT software comes with more than 100 categorized application tests, which greatly reduce the time required for characterizing new devices, processes and materials.

The application tests provided in the EasyEXPERT software library are conveniently categorized by device type and application. Sample categories include bipolar junction transistors (BJT), complementary metal-oxide-semiconductor (CMOS) transistors, nanotechnology structures and reliability tests. Although these application tests are ready to use as supplied, in some cases it may be necessary to customize them in order to meet the unique testing requirements of specialized technologies and devices.

Most of the input parameters for the EasyEXPERT application tests have upper and lower test limits. These limits are in-place to protect devices from damage that could occur from inadvertent mistakes such as incorrect keystrokes or operator entry

error. However, it is a relatively simple process for users to modify the input parameter ranges of the supplied EasyEXPERT application tests. Such modification may be necessary to test some of the newer and more exotic devices and process technologies.

This application note outlines the modification process by using the “Id-Vd” application test as an example. The note also shows how easily the upper and lower input parameter limits of this application test can be modified.

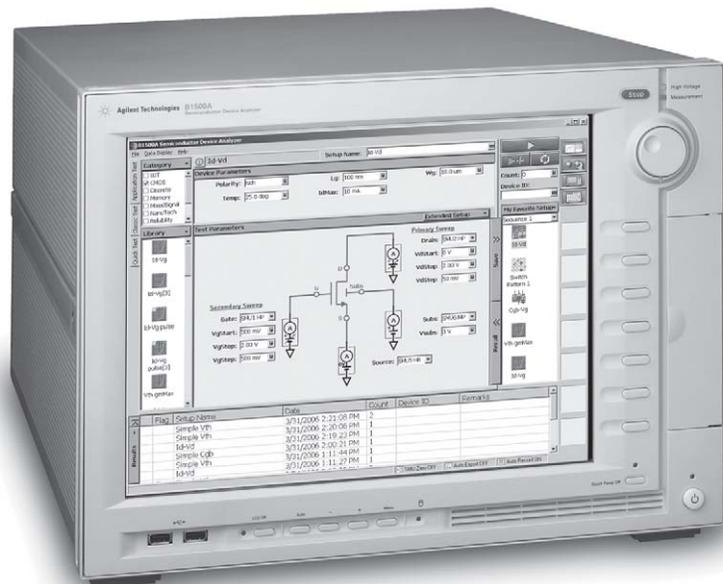

Agilent Technologies

## Modifying an existing application test definition

Figure 1 shows the error message that appears when the input value for an EasyEXPERT application test exceeds the pre-defined input parameter limits. The input parameter limit range can be easily expanded in two simple steps: opening the test definition window, and modifying the properties of the parameters. This process is explained in detail below.

### Opening the test definition window

The test definition window is used to define the test setup used in the application test definition. Figure 2 shows the three steps involved in opening the window:

1. Select the application test category that includes the application test definition to be opened (in this example the CMOS category).
2. Under Library, select the application test to be modified (in this example, the Id-Vd test).
3. In the Library pull-down menu, select "Open Definition of This Test..." The test definition window appears, as shown in Figure 3.

The Test Definition window provides three tabs to define the test setup. (Note that when the Test Definition window opens, the Test Specification tab is the default selection.)

- The Test Specification Tab defines the look and feel of the application test by specifying the test information, device parameter definitions, and test parameter definitions.
- The Test Contents Tab contains the test execution flow that is the essence of the test definition.
- The Test Output Tab specifies the data output and is generally only needed for certain types of very complicated tests.

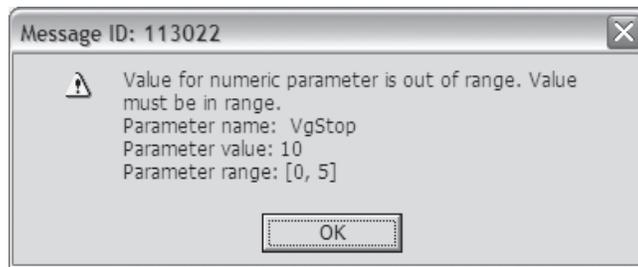


Figure 1. Input value error message.

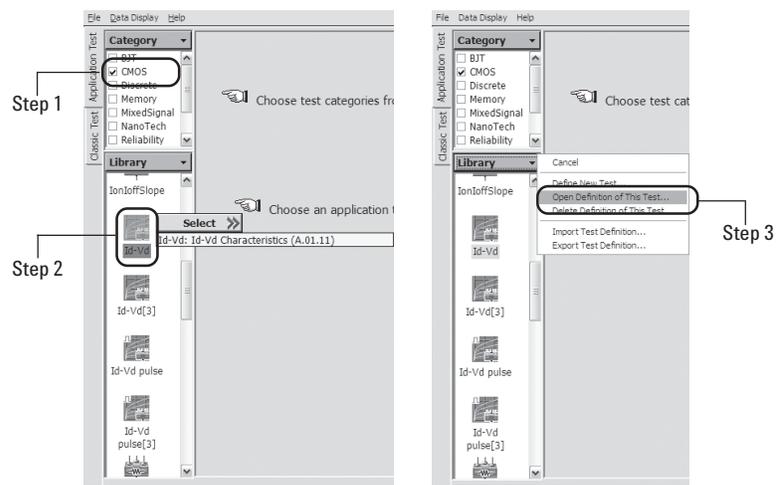


Figure 2. Steps required to open the Test Definition window.

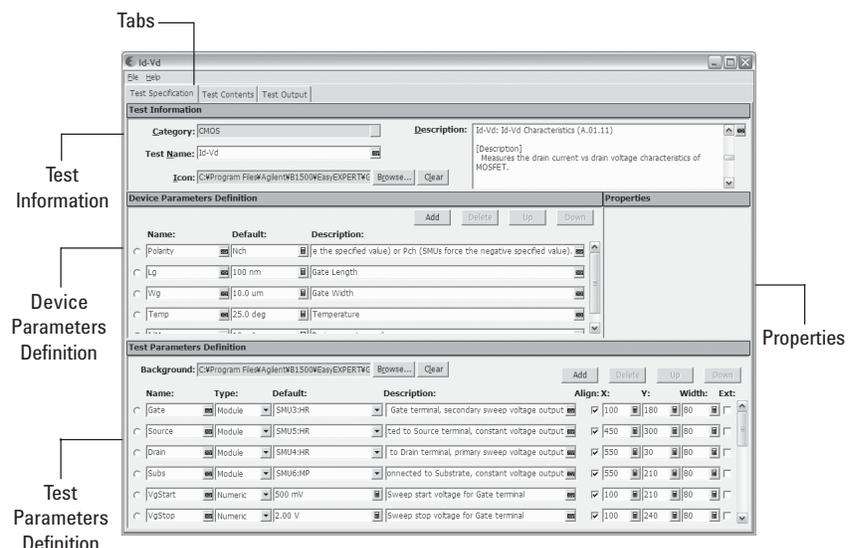


Figure 3. Test Definition window.

## Changing parameter properties

In this application note, the Test Specification setup is used as an example. Figure 3 shows the four setup areas under the Test Specification tab.

- Test Information
- Device Parameters Definition
- Test Parameters Definition
- Properties

In the Test Information area, the test name, the icon file name

(which appears in the Library area of the main window), and the description of the test are specified. The Device Parameters Definition and Test Parameters Definition area define the parameters used in the application test.

The Properties area is used to define the properties of the parameters of both the Device Parameters Definition area and the Test Parameters Definition area.

The relationship between the Test Specification setup area and the main window is shown in Figures 4 and 5. The default value in the Test Parameters Definition area appears as a default input parameter in the main window, and the properties of this input value can be set in the Properties area.

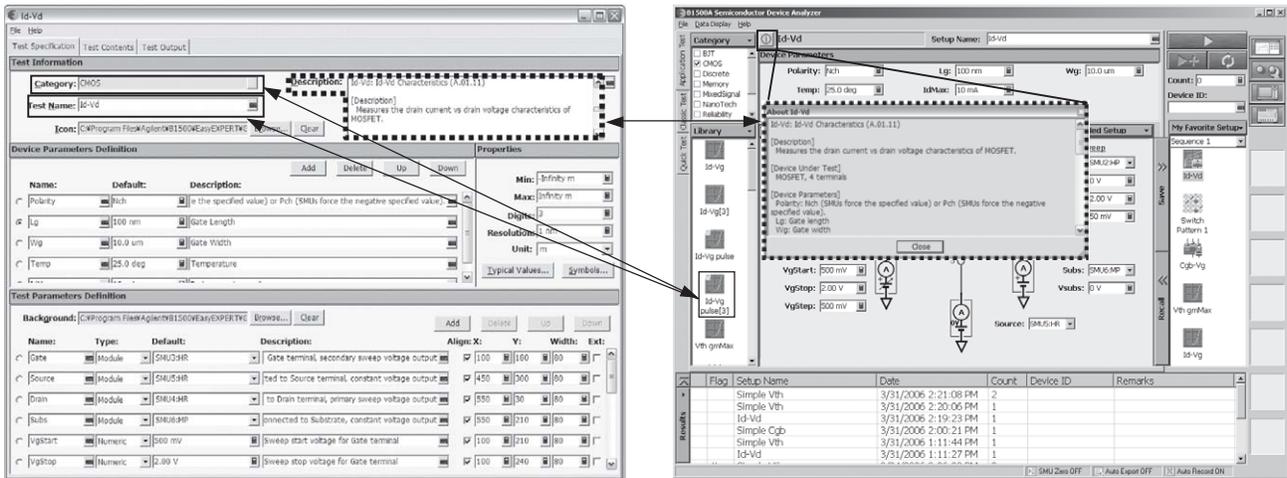


Figure 4. Relationship between the Test Specification window and the Main window with respect to Test Information.

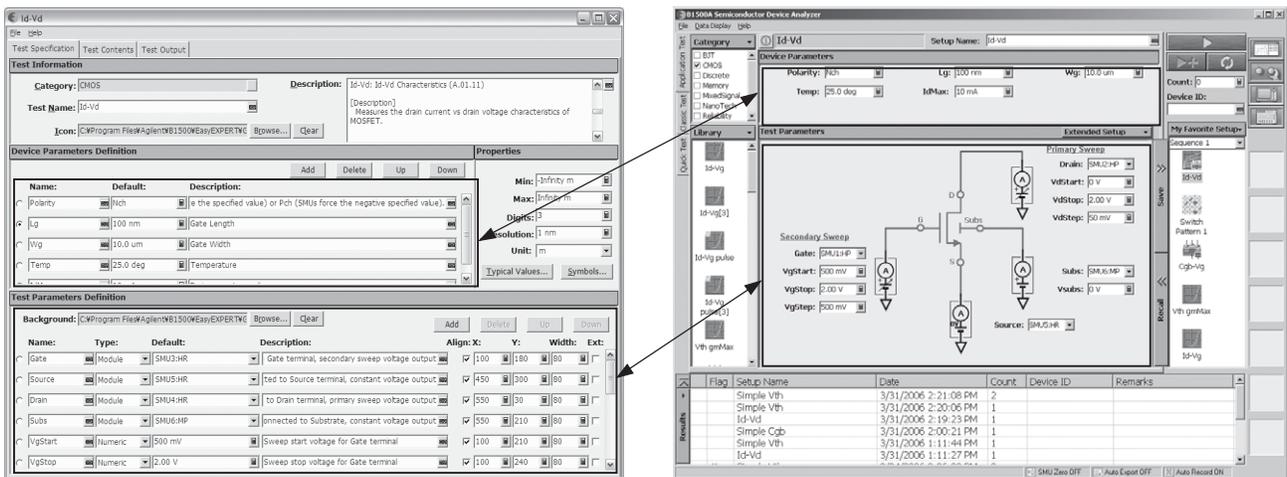


Figure 5. Relationship between the Test Specification window and the Main window with respect to the Device Parameters Definition and the Test Parameters Definition.

Before changing the parameters of a test definition, it is advisable to first save the test definition under another name. This prevents inadvertently overwriting the original application test. In this case, for example, the name

of the test definition could be changed from "Id-Vd" to "Id-Vd Mod".

In this example, the maximum allowable value of the input parameters VgStart, VgStop, VdStart,

and VdStop for the furnished Id-Vd application test was set at 5 V. Notice that when any of these parameters in the Test Parameter Definition area is selected, the properties of the input value appear in the Properties area.

## Changing parameter properties (continued)

Figure 6 shows how easy it is to increase the maximum value of the input parameter (in this case from 5 V to 10 V). Of course, this operation must be repeated for each of the input parameters to be modified.

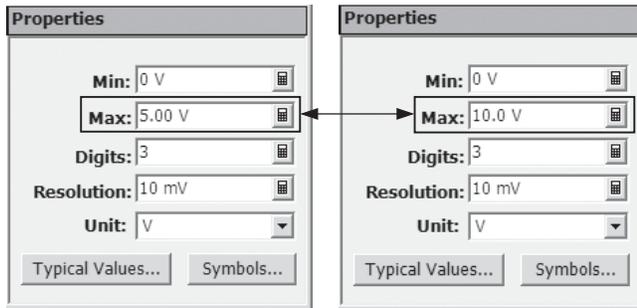


Figure 6. Increasing the maximum value of the input parameter in the Properties window.

Finally, the modified test definition must be saved by selecting the File > Save menu and then closed by the selecting the File > Close menu. Using this modified application test, it is now possible to input a value of up to 10 V into any of the VgStart, VgStop, VdStart, or VdStop input fields.

### Conclusion

Modifying the input parameter range of the furnished B1500A application tests is a simple operation, which makes it possible to test a greatly expanded set of devices and technologies.

For more information about Agilent and its products, go to [www.agilent.com](http://www.agilent.com).

For more information about Agilent Technologies semiconductor test products, applications, and services, visit our Web site: [www.agilent.com/go/semiconductor](http://www.agilent.com/go/semiconductor) or call one of the centers listed and ask to speak with a semiconductor test sales representative.

#### Americas

Brazil (11) 4197-3600  
Canada (French) 1 877 894-4414  
Canada (English) 1 800 447-8378  
Mexico 33 134-5841  
United States 1 800 447-8378

#### Asia/Asia Pacific

Australia 1 800 629-485  
China 1 800 276-3059  
Hong Kong 852 2599 7889  
India 91/11 690-6156  
Japan 0120 421-345  
Malaysia 1 800 880-780  
New Zealand 0 800 738 378  
Philippines 1 800 1651-0135  
Singapore 1 800 276-3059  
South Korea 080 778-0011  
Taiwan 0 800 047-662  
Thailand 1 800 2758-5822

#### Europe

Austria (01) 25 125-7183  
Belgium (0) 2 404-9380  
Denmark 080301040  
Finland 20 547-9999  
France (0) 825 010710  
Germany (0) 18 05 24-63 34  
Greece 20 547-9999  
Ireland 016158393  
Italy 02 92 60 8333  
Luxembourg (0) 2 404-9340  
Netherlands (0) 20 547-9999  
Poland 20 547-9999  
Russia 20 547-9999  
Spain 91 631 3383  
Sweden 020 120-9975  
Switzerland (Italian) (0) 2 92 60 8484  
Switzerland (German) (0) 1 735-9300  
Switzerland (French) (0) 825 010 700  
United Kingdom (0) 7004 222-222

#### Middle East

Israel 20 547-9999

Technical data subject to change without notice.

Microsoft and Windows are U.S. registered trademarks of Microsoft Corporation.

© Agilent Technologies, Inc. 2006  
Printed in USA September 21, 2006  
5989-5167EN