

Multi-channel signals with programmable inter-channel phase

This solution requires a C-size VXI cage, a control card, an E1420A counter and, if more than two E1440As are used, an E1366A switching unit.

Features and benefits

- Slave E1440A frequencies can be a multiple of master frequency.
- Channels can be independently modulated (AM or PM).
- 11-digit frequency resolution.
- Phase accuracy +/- 2 degree at 20 MHz (even better at lower frequencies due to counter's 200 ps time-interval resolution).
- Output waveforms need not be the same, and are selectable from:
 - sine (up to 21 MHz), square or triangle (up to 11 MHz), and ramp (up to 11 kHz). Minimum frequency is 1 uHz.
- 5 ppm stability, if E1440As are daisy-chained. Can be improved by using the counter reference.
- Independent amplitude 1 mVpp to 10 Vpp into 50 ohm. Option 001 provides 4 mVpp to 40 Vpp into 500 ohm.


Application example: Navigation Systems

Test of vehicle receivers used in Decca-type location systems requires a number of synthesizers to simulate the signals from a number of fixed transmitters. The frequencies, which are multiples of the master transmitter frequency, must not only be phase-locked, but also of programmable phase so that receiver performance can be verified for any vehicle position.


Setting up for the first time


After inserting the modules in the VXI-cage, the front panel connections shown in the following diagram must be made. Additionally, the counter's 10 MHz reference can be "daisy-chained" to all E1440As; this however is not essential, the VXI-internal CLK10 line can be used instead.

a) Two channels

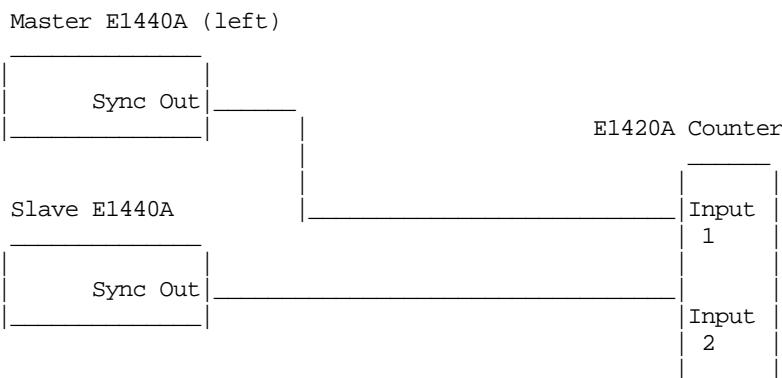

b) Three to five channels

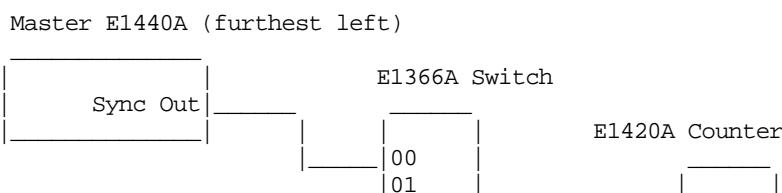

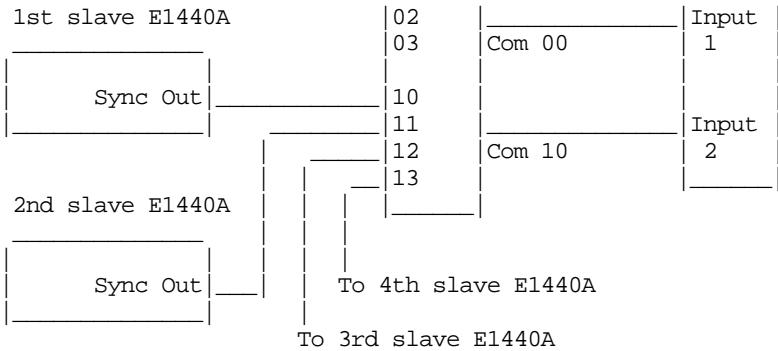

Try to keep the Sync Out path lengths as equal as possible. The same applies to the main outputs. Perform a phase measurement at the device and note any offset needed. With propagation times equalized, the phase accuracy lies in the range /-1 to /- 7 degree depending on waveform and amplitude mix, and frequency.

From here on, correct phase relationship is simply a matter of setting each slave to the required phase. Subsequently, whenever frequency, waveform or amplitude are changed, a phase-cal should be performed. If more than one counter is detected, the one with the lowest slot number will be taken.

Also, the current settings of the counter and switch are stored. This is to allow the counter to be used for other measurements. After the phase calibration, the previous counter settings are automatically recalled.

The calibration is done by the subprogram Sc_calibrate, which first measures the time delay between the positive slopes of the sync signal from the master device (which is used as a reference) and the sync signals from the slaves. It then calculates the phase error between master and slave and adjusts each slave so that all channels are in phase with the master.

After calibration, the program sets the different E1440A's to the desired phase values. Then, as mentioned above, counter and switch are returned to their previous settings.

Automation

UNSUPPORTED programs are attached:

1. PHASECAL: provides a user interface and phase-calibrates automatically.
2. ERRORHANDLING: a utility for use in any application where self-test is to be implemented.

The programs are in HP Basic and stored as ASCII files (use the HP Basic command GET to load the file).

PHASECAL implements phase calibration for up to five HP E1440As. If a daisy-chained reference signal is used instead of VXI line CLK10, change line 109 from:

```
109 OUTPUT Hpib E1440(I,2);":SOURCE:ROSC:SOURCE CLK10"
! CLK10 is ref
```

to:

```
109 OUTPUT Hpib E1440(I,2);":SOURCE:ROSC:AUTO ON"
! Daisy chain ref
```

Initially, the routine detects the cards in the VXI-cage (SUB Sc_getdev) and assigns the E1440A with the lowest slot number as master, the one with the next higher slot number will be slave 1, and so-on. If more than one E1420A counter is detected, the one with the lowest slot number will be taken.

Also, the current settings of the counter and switch are stored.

This is to allow the counter to be used for other measurements.

The calibration is done by the subprogram Sc_calibrate, which first measures the time delay between the positive slopes of the sync signal from the master device (which is used as reference) and the sync signals from the slaves. It then calculates the phase error between master and slave and adjusts each slave so that all channels are in phase with the master.

After calibration, the program sets the different E1440's to the desired phase values, and returns the counter and switch to their previous settings.

```
1      ! PHASE CALIBRATION UTILITY (IN RMB) FOR A MASTER E1440A
2      ! WITH UP TO FOUR SLAVE E1440As.
3      !
4      ! E1420A COUNTER MUST BE INSTALLED IN THE SAME MAINFRAME.
5      !
6      ! IF THERE IS MORE THAN ONE SLAVE, A PROGRAMMABLE CO-AX
7      ! SWITCH WILL ALSO BE NEEDED. THIS PROGRAM USES THE
8      ! E1366A SWITCH
9      !
10     !
11     !
12     REAL Counter      ! HPIB-address of E1420 e.g. 71605
13     REAL Switch       ! HPIB-address of Switchbox
14     REAL Master        ! HPIB-address of master E1440
15     REAL Frequency     ! Frequency of master E1440
16     REAL Master_phase ! Phase of master E1440 after calibration
17     REAL Slave(1:4)    ! HPIB-addresses of slave E1440's, 0 for
                           unused slaves
18     INTEGER Slave_multi(1:4)
19     REAL Slave_phase(1:4) ! Slave phase after cal
20     REAL Error          ! Return value: 0=cal ok, 1=timeout
21     INTEGER Pm_cal      ! 0: CALIBRATION WILL BE DONE FOR PM BY
                           !      SWITCHING OFF/ON PM INPUTS
22                           !      THIS MAY CAUSE FOR SQUAREWAVES A PHASE
23                           !      SHIFT OF 180 DEGREES
24                           !<>0: FOR SQUAREWAVES WITH PM, THE PROGRAM WILL
25                           !      CALIBRATE WITH PM SWITCHED ON AND ASK
26                           !      TO DISCONNECT/CONNECT THE CABLES TO THE
27                           !      PM INPUTS. THIS PROTECTS FROM THE PHASE
28                           !      SHIFT, BUT NEEDS MANUAL MODIFICATIONS OF
29                           !      THE TEST CABLE CONNECTIONS
30                           !
31     !
32     Frequency=1500
33     Slave_multi(1)=1
34     !
35     REAL Hpib ! incl sec addr. Used only for Sc_getdev subpgm
36     Hpib=71600 !      HAS TO BE CHANGED TO VALID ADDRESS
37     CALL Sc_getdev(Hpib,Counter,Switch,Master,Slave(*))
                           !      assign dev addresses
38     !CALL
39     !c_calibrate(Counter,Switch,Master,Frequency,
                           Master_phase,Slave(*),
40     !Slave_multi(*),Slave_phase(*),Error,Pm_cal)
41     END
42     !
43     =====
44     SUB Sc_getdev(Hpib,Counter,Switch,Master,Slave(*))
                           ! CHECK DEV ADDRESSES
45     !      this subprogram is only used to show how the
                           configuration of the VXI
46     !      -mainframe can be detected automatically. It is
                           not needed for calibration
47     INTEGER I,Devnumber,Count,E1440a,E1420a,Sbox
48     !REAL Mfg,Dummy,La(1:13),E1440(1:5,1:2),Slot,Dev,
49     !!Switchbox(1:3,1:2),E1420(1:3,1:2)
50     DIM Dev$[20],Dummy$[200],Dlad$[50]
```

```

51 Counter=0
52 IF NOT Hpib THEN SUBEXIT
53 ON TIMEOUT INT(Hplib/10000),5 GOTO Timeout_error
54 Dev=Hpib
55 OUTPUT Hpib;":VXI:CONF:DNUM?"
56 ENTER Hpib;Devnumber
57 OUTPUT Hpib;":VXI:CONF:DLAD?"
58 ENTER Hpib;Dlad$
59 FOR I=1 TO Devnumber
60 La(I)=VAL(Dlad$)
61 Dlad$=Dlad$[POS(Dlad$,"") 1,LEN(Dlad$)]
62 OUTPUT Hpib;":VXI:CONF:DLIS? "&VAL$(La(I))
63 ENTER Hpib;Dummy,Mfg,Dummy,Slot,Dummy$
64 IF Mfg=4095 THEN ! manufacturer hp ?
65 La(I)=INT(La(I)/8)
66 Dev=Hpib La(I)
67 OUTPUT Dev;"*IDN?"
68 ENTER Dev;Dummy$
69 Dummy$=Dummy$[POS(Dummy$,"") 1,LEN(Dummy$)]
70 Dummy$=Dummy$[1,POS(Dummy$,"")-1]
71 SELECT Dummy$
72 CASE "E1440A"
73 E1440a=E1440a 1
74 Count=Count 1
75 IF Count<6 THEN
76   E1440(Count,1)=Slot
77   E1440(Count,2)=La(I)
78 END IF
79 CASE "E1420A"
80 E1420a=E1420a 1
81 E1420(E1420a,1)=Slot
82 E1420(E1420a,2)=La(I)
83 CASE "SWITCHBOX","E1472A"
84 Sbox=Sbox 1
85 Switchbox(Sbox,1)=Slot
86 Switchbox(Sbox,2)=La(I)
87 CASE ELSE
88 END SELECT
89 END IF
90 NEXT I
91 IF Count THEN
92   !!MAT SORT E1420(*,1)
93   !!MAT SORT Switchbox(*,1)
94 FOR I=3 TO 1 STEP -1
95   IF E1420(I,2) THEN
96     Counter=Hpib E1420(I,2)
97   END IF
98   IF Switchbox(I,2) THEN
99     Switch=Hpib Switchbox(I,2)
100  END IF
101 NEXT I
102 !!MAT SORT E1440(*,1)
103 Count=0
104 FOR I=1 TO 5
105   IF E1440(I,2) THEN
106     Count=Count 1
107     IF Count=1 THEN Master=Hpib E1440(I,2)
108     IF Count>1 THEN Slave(Count-1)=Hpib E1440(I,2)
109     OUTPUT Hpib E1440(I,2);":SOURCE:ROSC:SOURCE CLK10"
           ! CLK10 is ref
110   END IF
111 NEXT I
112 END IF
113 IF E1420a=0 THEN PRINT "CONFIG ERROR: No E1420 cntr"
114 IF Sbox=0 AND E1440a>1 THEN
115   PRINT "CONFIG MESSAGE: No Switchbox"
116 END IF
117 IF E1440a<2 THEN PRINT "CONFIG ERROR: No E1440"
118 OFF TIMEOUT
119 SUBEXIT

```

```

120 Timeout_error:!
121 OFF TIMEOUT
122 !!PRINT "ERROR: No device "&VAL$(Dev)&
123 SUBEND !=====
124 !!SUB Sc_calibrate(Counter,Switch,Master,Frequency,
125 Master_phase,Slave(*),
126 !!INTEGER Slave_multi(*),REAL Slave_phase(*),Error,
127 INTEGER Pm_cal)
128 REAL Master_pm,Slave_pm,Test1,Test2,J,Slave_frequency,Fault
129 DIM Master_wave$[15],Slave_wave$[15]
130 INTEGER I
131 Error=1
132 IF NOT Master OR NOT Counter THEN SUBEXIT ! no master or
133 counter addr
134 IF Master<10000 OR Counter<10000 THEN SUBEXIT
135 ! incomplete addr
136 IF Frequency>2.1E 7 THEN SUBEXIT ! Frequency limit
137 ON TIMEOUT INT(Master/10000),7 GOTO No_count
138 !timeout? ->abort
139 OUTPUT Master;"":FREQ:FIX "&VAL$(Frequency)&"HZ;
140 :SOURCE:PM:STATE?"
141 ! check master pm
142 ENTER Master;Master_pm
143 OUTPUT Master;"":SOURCE:FUNCTION:SHAPE?
144 ! check master waveform
145 ENTER Master;Master_wave$
146 IF Master_wave$="DC" THEN SUBEXIT ! no calibration for dc
147 OUTPUT Counter;"*SAV 9" ! save counter setup
148 !!OUTPUT Counter;"":INP1:ROUTE SEP;:SENSE1:EVENT:SLOPE
149 !!POS;:SENSE2:EVENT:SLOPE POS;:INPUT1:COUP DC;:INPUT2
150 !!!:COUP DC;:INP1:IMP 50;:INP2:IMP 50"
151 !!OUTPUT Counter;"":SENSE1:EVENT:LEVEL:AUTO OFF;
152 :SENSE1:EVENT:LEVEL
153 !!!:ABS 1.5V;:SENSE2:EVENT:LEVEL:AUTO OFF;
154 :SENSE2:EVENT:LEVEL:ABS 1.5V"
155 IF (Switch MOD 10000) THEN OUTPUT Switch;"*SAV 9;
156 :ROUT:CLOS (@100)"
157 !!save mux settings, switch mux to connect master to
158 counter input 1
159 ON TIMEOUT INT(Counter/10000),7 GOTO No_cal
160 IF (Master_wave$<>"SQUARE") OR Master_pm<>1 OR
161 Pm_cal=0 THEN
162 OUTPUT Master;"":SOUR:PM:STAT OFF"
163 Test1=0 ! output has normal phase during calibration
164 ELSE ! select desired and necessary calibration
165 Test1=180! output has inverted phase during calibration
166 PRINT "CALIBRATION MESSAGE: Please disconnect cable from
167 PM input"
168 !!!ON KBD ALL GOTO !152
169 GOTO 151 ! wait for user action
170 !!OFF KBD
171 END IF
172 IF Master_phase<>Test1 THEN
173 FOR J=Master_phase TO Test1 STEP (Test1-Master_phase)/15
174 !! ! omit phase shift below 25 kHz
175 OUTPUT Master;"":SOUR:PHAS "&VAL$(PROUND(J,-1))&" DEG"
176 NEXT J
177 END IF
178 FOR I=1 TO 4
179 IF Slave(I) AND ((I=1) OR (Switch MOD 100)) THEN
180 ! slave on setup ?
181 !!IF (Switch MOD 10000) THEN OUTPUT Switch;"":rout
182 :clos (@11"&VAL$(I-1)&")
183 !! "Slave_frequency=Frequency*Slave_multi(I)
184 ! calculate new slave frequency
185 OUTPUT Slave(I);"":FREQ:FIX "&VAL$(Slave_frequency)&"HZ;
186 :SOURCE:PM:STATE?"
187 ENTER Slave(I);Slave_pm ! check slave for pm
188 OUTPUT Slave(I);"":SOURCE:FUNCTION:SHAPE?

```

```

173    ENTER Slave(I);Slave_wave$      !  check slave waveform
174    IF Slave_wave$<>"DC" AND Slave_frequency<2.1E 7 THEN
175    !! !  no calibration for dc or frequencies above 21MHz
176    IF (Slave_wave$<>"SQUARE") OR Slave_pm<>1 OR Pm_cal=0
177        THEN
178            OUTPUT Slave(I);":SOUR:PM:STAT OFF"
179        Test2=180
180    ELSE
181        Test2=0
181    PRINT "CALIBRATION MESSAGE: Please disconnect
181                  cable from PM input"
182    !! "at slave"&VAL$(I)&" device ("&VAL$(Slave(I))&")
182                  then press any key"
183    !!ON KBD ALL GOTO 176
184    !! GOTO 175          !  wait for user action
185    !!OFF KBD
186    END IF
187    IF Slave_phase(I)<>(180-Test2) THEN
188        FOR J=Slave_phase(I) TO 180-Test2 STEP
188            (180-Slave_phase(I))/15
189    !!! omit phase shift below 25 kHz for phase changes
189            > 25 deg (squarewave)
190        OUTPUT Slave(I);":SOUR:PHAS"&VAL$(PROUND(J,-1))&" DEG"
191        NEXT J
192    END IF
193    !
194    CALL Sc_measure(Counter,Master,Slave(I),Test2,
194                  Slave_frequency,Fault)
195    !
196    !!IF ABS(Fault-180)<179.5 THEN OUTPUT Slave(I);":SOUR:
196                  PHAS "&VAL$(
197                  !(Fault)&" DEG;:SOURCE:PHASE:REFERENCE"
198    IF Slave_phase(I) THEN
199        FOR J=0 TO Slave_phase(I) STEP (Slave_phase(I))/15
200    ! omit phase shift below 25 kHz
201        OUTPUT Slave(I);":SOUR:PHAS "&VAL$(PROUND(J,-1))&
201                  " DEG"
202        NEXT J
203    END IF
204    OUTPUT Slave(I);":SOUR:PM:STAT "&VAL$(Slave_pm)
205    IF (Slave_wave$="SQUARE") AND Slave_pm=1 AND Pm_cal<>0
205        THEN
206    !! PRINT "CALIBRATION MESSAGE: Please connect cable to
206                  PM input at
207    !!slave"&VAL$(I)&" device ("&VAL$(Slave(I))&) then
207                  press any key"
208    !! ON KBD ALL GOTO 197
209    GOTO 196          !  wait for user action
210    !! OFF KBD
211    END IF
212    END IF
213    END IF
214    NEXT I
215    IF Test1<>Master_phase THEN
216        FOR J=Test1 TO Master_phase STEP (Master_phase-Test1)/15
217    ! omit phase shift below 25 kHz for changes > 25 deg (only
217                  for squarewave)
218        OUTPUT Master;":SOUR:PHAS "&VAL$(PROUND(J,-1))&" DEG"
219        NEXT J
220    END IF
221    OUTPUT Master;":SOUR:PM:STAT "&VAL$(Master_pm)
222    IF (Master_wave$="SQUARE") AND Master_pm=1 AND Pm_cal<>0
222        THEN
223    !! PRINT "CALIBRATION MESSAGE: Please connect cable to
223                  PM input at
224    !!master device ("&VAL$(Master)&"), then press any key"
225    !! ON KBD ALL GOTO 212
226    GOTO 211          !  wait for user action
227    !!OFF KBD
228    END IF

```

```

229 OUTPUT Counter;"*rcl 9"           ! re-store counter setup
230 IF (Switch MOD 10000) THEN OUTPUT Switch;"*rcl 9"
                                ! re-store mux setup
231 OFF TIMEOUT
232 Error=0      ! no error occurred
233 SUBEXIT
234 No_cal:!
235 ON TIMEOUT INT(Counter/10000),7 GOTO No_count
236 ! if device timeout then abort
237 OUTPUT Counter;"*rcl 9"           ! re-store counter setup
238 IF (Switch MOD 10000) THEN OUTPUT Switch;"*rcl 9"
                                ! re-store mux setup
239 No_count:      !
240 OFF TIMEOUT      ! calibration not successful, timeout
241 SUBEND
242 =====
243 SUB Sc_measure(Counter,Master,Slave,Test2,Frequency,Fault)
244 REAL Resolution,Measure(1:3),J,Tout
245 IF Frequency>2000 THEN
246 ! select measurement resolution of counter depending on
               expected timeinterval
247 Resolution=1.E-10
248 ELSE
249 Resolution=1.E-9
250 END IF
251 Tout=3/Frequency 5
252 Sc_getdelay(Frequency,Resolution,360,Counter,Tout,
               Measure(1))
253 Sc_getdelay(Frequency,Resolution,360,Counter,Tout,
               Measure(2))
254 !!IF (ABS(Measure(2)-Measure(1))>1.5) AND ((ABS
               (Measure(1)-180)<179)
255 !! OR (ABS(Measure(2)-180)<179)) THEN
               ! both values in tolerance?
256 ON TIMEOUT INT(Counter/10000),5 GOTO End
257 FOR J=180-Test2 TO Test2 STEP (Test2/5-18)
258 ! omit phase shift below 25 KHz for phase changes >
               25 deg on squarewave signals
259 OUTPUT Slave;":SOUR:PHAS "&VAL$(PROUND(J,-1))&" DEG"
260 NEXT J
261 WAIT .3
262 Sc_getdelay(Frequency,Resolution,540,Counter,Tout,
               Measure(3))
263 !!IF (ABS(Measure(2)-Measure(3))>2) AND ((ABS
               (Measure(2)-180)<178.5) OR
264 !! (ABS(Measure(3)-180)<178.5)) THEN
               ! compare second with third measurement
265 Measure(3)=Measure(1)
266 Measure(1)=Measure(3)
267 Sc_getdelay(Frequency,Resolution,540,Counter,Tout,
               Measure(3))
268 !!IF (ABS(Measure(1)-Measure(3))>3) AND ((ABS
               (Measure(1)-180)<178) OR
269 !! (ABS(Measure(3)-180)<178)) THEN 246
               ! last two measurements in tolerance?
270 Measure(2)=Measure(3)
271 ELSE
272 Measure(1)=Measure(3)
273 END IF
274 FOR J=Test2 TO 180-Test2 STEP (18-Test2/5)
               ! omit phase shift
275 ! below 25 KHz for phase changes > 25 deg on squarewave
               signals
276 OUTPUT Slave;":SOUR:PHAS "&VAL$(PROUND(J,-1))&" DEG"
277 NEXT J
278 END IF
279 IF Measure(1)>355 AND Measure(2)<5 THEN Measure(1)=
               Measure(1)-360
280 IF Measure(2)>355 AND Measure(1)<5 THEN Measure(2)=
               Measure(2)-360

```

```

282 Fault=PROUND((Measure(1) Measure(2))/2,-1)
          ! thats the phase error
283 BEEP 200,.05      ! MEASUREMENT DONE
284 End:OFF TIMEOUT
285 SUBEND
286 =====
287 SUB Sc_getdelay(Frequency,Resolution,Degree,Counter,Tout,
                     Measure)
288 OFF TIMEOUT
289 IF Tout<32 THEN
290 ! if calibration needs longer than 32.767 seconds, the
291 ! timeout command can't be used to avoid a hang-up
292 ON TIMEOUT INT(Counter/10000),Tout GOTO T_out
293 ELSE
294 !! ON TIME Tout GOTO T_out
295 END IF
296 OUTPUT Counter;"":MEASURE1:TINTERVAL? 1,"&VAL$(Resolution)
297 ENTER Counter;Measure
298 Measure=(PROUND(Measure*Frequency*360,-1) Degree) MOD 360
299 T_out:OFF TIMEOUT
300 !!OFF TIME
301 SUBEND

```

Part 4.

```

10 !E1440A Self-cal error-handling routine.
20 !Prints "self-cal OK" or, if there is a fault, the
           self-cal results.
30 !A timeout recovers system control if the E1440A fails
           to respond.
40 CLEAR SCREEN
50 ASSIGN @Fg TO 71611
60 ABORT 7
70 CLEAR 7
80 CLEAR @Fg
90 !
100 Cal$=" 9"
110 !
120 !
130 OUTPUT @Fg;"*RST;:STATUS:PRESET;*CLS"
140 OUTPUT @Fg;"":VOLT 5V" ! This statement causes self-cal
150 ON TIMEOUT 7,3 GOTO Timeout
160 OUTPUT @Fg;"":CAL?" ! Self-cal data requested
170 ENTER @Fg;Cal$ ! Self-cal data uploaded
180 IF Cal$=" 0" THEN
190     PRINT "Self-cal ok"
200 ELSE
210     PRINT "Self-cal error ";Cal$;"see Manual p 5-9"
220 END IF
230 GOTO End
240 !
250 Timeout:PRINT "Timeout, E1440A doesn't respond within normal self-cal time (
3 s)"
260 !
270 End:LOCAL @Fg
280 !
290 END

```